

(19) World Intellectual Property  
Organization  
International Bureau



(43) International Publication Date  
10 June 2004 (10.06.2004)

PCT

(10) International Publication Number  
**WO 2004/047710 A1**

(51) International Patent Classification<sup>7</sup>: **A61G 10/02**,  
10/00

(21) International Application Number:  
PCT/AU2003/001540

(22) International Filing Date:  
19 November 2003 (19.11.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
2002952811 22 November 2002 (22.11.2002) AU

(71) Applicant (for all designated States except US): **OXY-  
GEN THERAPY INTERNATIONAL PTY LTD**  
[AU/AU]; Suite 7, Glenham Plaza, 17 Carp Court, Bun-  
dall, QLD 4217 (AU).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **MEYER, Allan,**

**Dolph** [AU/AU]; 8 Hartree Court, Cherrybrook, NSW  
2126 (AU). **BERRY, Norman, Micheal** [AU/AU]; 7  
Paling Street, Thornleigh, NSW 2120 (AU). **DAVIDSON,  
Martin** [AU/AU]; 408/1 Georgina Street, Newtown, NSW  
2042 (AU).


(74) Agent: **GRANT, Paul, Ainsworth**; P.O. Box 7460, Fisher,  
ACT 2611 (AU).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU,  
AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR,  
CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD,  
GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR,  
KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN,  
MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU,  
SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA,  
UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (*regional*): ARIPO patent (BW, GH,  
GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),  
Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),

[Continued on next page]

(54) Title: **HYPERBARIC THERAPY CAPSULE**

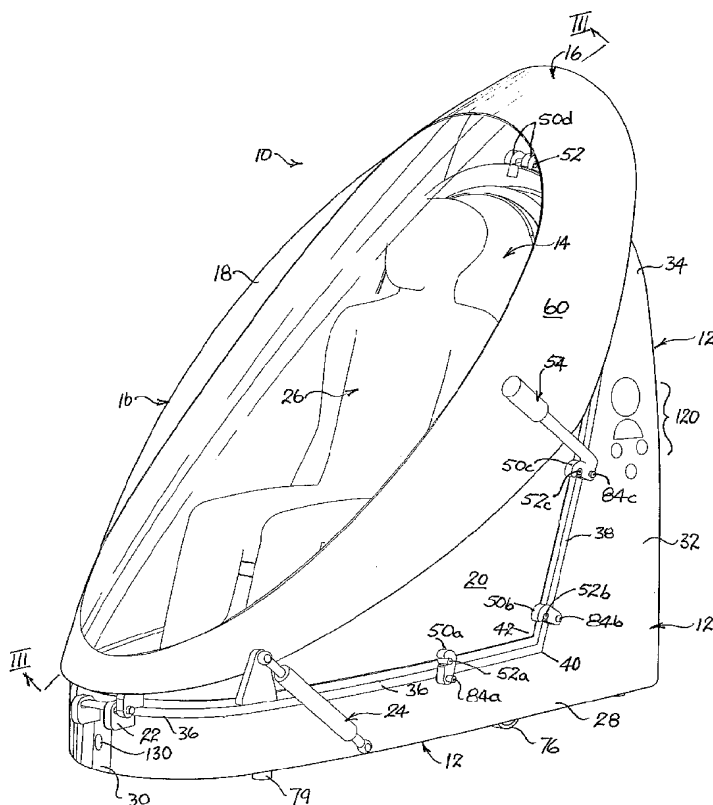

(57) Abstract: A hyperbaric capsule (10) has a base (12) forming a seat (14) that can be enclosed by an elongate oval canopy (16) having a large transparent window (18) formed therein. The bottom of the front of the canopy (16) is pivotally attached to the front of the base (12) by a hinge assembly (22) and can be locked in the closed position on the base by a plurality of latches (50a - 50d) that are conjointly operated by an external lever (54) and an internal lever (56, not shown in Figure 1). The weight of the canopy upon opening is borne by a pair of side gas or spring struts (24).



European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

**Published:**

— *with international search report*

**TITLE:** HYPERBARIC THERAPY CAPSULE

**TECHNICAL FIELD**

This invention relates to a chamber suitable for use by a person for hyperbaric  
5 oxygenation for therapy, prophylaxis or general health improvement. It is  
particularly, though not exclusively, concerned with a hyperbaric capsule suitable  
for use by one person at home, or for use by a clinic for the treatment individual  
clients. The capsule may be used with or without oxygen enrichment of air  
breathed by the user.

10

This invention also relates to methods for operating such capsules to ensure  
efficacy and safety.

**BACKGROUND TO THE INVENTION**

15 Hyperbaric chambers known in the art are commonly designed for the  
recompression of divers to mitigate gas embolism, the treatment of patients in a  
hospital or clinic environment and for diver or athlete training. In much of the art  
known to the applicant, hyperbaric chambers are massive and complex devices  
that require expert attendant staff. Such chambers are therefore not suited for  
20 home use by individuals without attendants. Moreover, since expert staff will be in  
attendance while the hyperbaric chambers of the art are in use, no provision is  
made for the user or patient to open the chamber from within so that he or she  
can exit without assistance.

25 In many hyperbaric chambers for use in the clinical environment the patient is  
required to lie prone in a tube. Indeed, it is important in recompression chambers  
for the patient to be prone and inclined head-down at an angle of about 30  
degrees. This results in the massive construction typical of many such chambers.  
[See, for example, US patents 4, 727,870 to Krasel, 5,433,334 to Reneau and  
30 6,354,457 to Aaron, and US design patents 346,864 to Reneau and 415,278 to  
Bowman.] However, it is also important that recompression chambers be capable  
of being transported to a diver with the bends and rapidly deployed on site.  
Relatively compact chambers suitable for transport by truck or plane are therefore  
known in the art. [See, for example, US patents 4,811,729 to Sands et al,

5,378,093 to Santi and 6,321,746 to Schneider. For relatively modest recompression pressures, portable inflatable chambers with flexible walls are also known in the art. [See, for example, the above US patents to Santi and Schneider as well as US patents 5,109,837 and 5,398,678 and to Gamow, 5,255,673 to  
5 Cardwell and 5,360,001 to Brill.]

The traditional design of a hyperbaric chamber for use in hospitals and clinics is a cylinder with a round door at one end through which the patient can be introduced in the prone position. Such a design appears to have been dictated by the need to  
10 minimize the area of the end door so that the force on the door is modest even when the chamber is fully pressurized. Nevertheless, many such chambers have the appearance and claustrophobic feel of totally enveloping 'iron lungs' that prevent the patient from moving significantly – let alone sitting up – and that allow visual contact with the operators through small portholes only. [See, for example,  
15 US patent to Krasel above.] The fact that there is generally no way that the user can open the chamber from within exacerbates the natural claustrophobic anxiety associated with enclosure in such a confined space.

Nevertheless, the prior art does disclose designs for hyperbaric chambers that  
20 permit the patient to be seated. US patent 5,327,904 to Hannum and US patent 6,352,078 to Harvey disclose short cylindrical chambers of sufficient diameter to accommodate a seated person. In the former case a flat door is fitted into the cylindrical shell and in the latter case the door is set into one end. In both cases, however, the doors open inwards (to enhance strength and facilitate sealing under  
25 pressure). Since the open door must allow the user entry and, after entry, must clear the seated user as it is being closed, the size of the chamber still needs to be substantial. Hannum nevertheless notes that an important feature of his chamber is that can be made sufficiently compact to fit through double (hospital) doors. Again, both chambers require the attendance of a skilled operator  
30 throughout the treatment of the patient or user, including the opening of the door to permit entry and egress at the start and end of the procedure. Thus neither chamber is suited to home use, for installation in a normal house or for use by a person without assistance.

Finally, it is to be noted that US patent 4,50a - 50d9,513 to Lasley discloses a 'hyperbaric chamber' that appears to be suitable for home use by a person without assistance. However, the device is a bag into which the user climbs like a pair of angler's waders, securing the opening around the upper part of the body (below the shoulders and not including the arms) to form a seal. The bag is then inflated with oxygen-enriched air. Obviously this device is not, in fact, a hyperbaric chamber in the normal sense – that is, one intended for pulmonary oxygenation.

## OUTLINE OF THE INVENTION

- From one aspect, this invention is a hyperbaric capsule that has (i) an elongate base molding which incorporates the form of a chair and which extends forward from the chair at user foot level and upward above user head level at the back of the chair and (ii) an elongate canopy that extends forward and downward from above user head level. The canopy has an elongate transparent window and is moveable between an open position, where a user can freely move to and from the chair via the side of the capsule, and a closed position where a seated user is fully enclosed by the canopy and base, which together form a hyperbaric chamber. The base molding and the canopy define respective seal-lines that cooperate to form an air-tight seal between the base and the canopy when the canopy is closed. Preferably, the canopy and its window have convex external surfaces that are curved in both the front-to-back and the side-to-side directions, the window preferably extending from at least user head level to the level of the seat of the chair.
- The capsule is preferably fitted with latches for securing the canopy to the base at a plurality of points about its periphery, the latches preferably being operable in unison by an actuator located within the capsule and an actuator located outside the capsule. The latches may take the form of hooks mounted on the ends of shafts, which extend transversely through the base, and coacting latch pins mounted on the canopy. The arrangement may be such that outward movement of the canopy sides under pressure is resisted by the hooks and their shafts. However, it is also envisaged that the sides of the canopy may fit within the periphery of the base so that outward movement of the canopy sides is also resisted directly by the periphery of the base. Preferably, where hooks are used

as the latches, they have an over-center action whereby an opening force applied to the canopy acts to bias the hooks further toward their secure or closed positions, thereby inhibiting operation of the actuators to effect the opening of the canopy while it is under pressure.

5

The chair will normally comprise a back adapted to support the back of the user at a comfortable angle to the vertical and a seat adapted to support the buttocks of the user at a comfortable angle to the horizontal. The base of the capsule preferably includes a floor in front of and below the chair seat adapted to support and accommodate the feet of a seated user. The base, the floor and the seat and back of the chair are preferably all molded integrally from fiber-reinforced plastics material to incorporate a metal base frame to withstand the operating pressure of the capsule. The peripheral base seal-line is preferably made up of (i) a first generally horizontal U-shape periphery that extends from the seat on each side of the chair and around the front foot area of the base, and (ii), a second generally vertical inverted U-shape periphery that extends from below the seat on each side and over the back of the chair. The first and second U-shape peripheries of the base join at an angle below the seat to complete the base seal line. The canopy has downwardly extending triangular side portions that have a corresponding angle so that they will fit into the join of the first and second U-shape peripheries of the base.

With this form of canopy and base, it is preferable for multiple hook-form latches to be arranged around the join between the two U-shape peripheries of the base and for their corresponding latch pins to be arranged in the triangular portions of the canopy, so that lateral movement of the side portions under pressure is resisted in the manner noted above

To doubly ensure that the canopy cannot be flung open forcefully by premature release of the latch means, a pressure-operated lock may be fitted to prevent operation of the actuator as long as pressure within the capsule is greater than that outside. Preferably, this lock is operable within the capsule so that it can be moved manually by a person in the capsule in the event that it does not automatically release after the capsule is depressurized.

The canopy is preferably of a dished elongate oval shape that (when closed) encompasses the base from the floor area to the top of the chair back. It can be formed from a thick sheet of highly transparent thermoplastic material by applying heat and fluid pressure – without the need for a mold – to generate the desired shape. Since the transparent portion of the canopy can extend in the front-to-back direction from over the head to near the feet of a seated user and, in the side-to-side direction, over the width of the user's body, there is little sense of claustrophobia. An edging of fiber-reinforced plastic material can be applied to the periphery of the canopy to form the canopy seal line and to mount the latch pins and other fittings (such as hinges and gas struts).

The canopy is preferably hingedly attached to the base at the front of the foot area so that it can pivot forwards to allow ready ingress and egress of the user from the at least one side of the capsule. The weight of the canopy may be supported in the open or partially open position by the use of gas struts or the like located at the front of the canopy on each side near of the floor. A flexible rubber-like sealing ring can be readily fitted to the periphery of the canopy and/or that of the base to ensure a substantially hermetic seal therebetween along the respective seal-lines of the base and the canopy, when the canopy is closed.

It will be appreciated that a capsule of the type described can be readily made to be small enough to fit through the standard doorways of a normal domestic dwelling and to be handled by one or two installers, particularly if the base is provided with wheels. However, because of its small size and volume, it is desirable that there be adequate provision for heat and CO<sub>2</sub> removal. This may be achieved by ensuring sufficient flow of pressurized air through the capsule while it is in use. The pressurized air may be conditioned to user-controlled temperature and humidity. Additionally, heat-exchanger means may be provided to cool the base or chair of the capsule.

If oxygen supplementation is required, it will generally be most safe and economical for the user to employ an oxygen mask while sitting in the capsule. Alternatively, the input air to the capsule can be enriched with oxygen.

With single-person use in mind, it is desirable that pressure, temperature and air/O<sub>2</sub> flow controls and/or indicators are located conveniently within the capsule, preferably on the base thereof or on a lower portion of the canopy. Various  
5 audible and/or visual alarms may also be desirable; for example, a power-failure alarm, an excess temperature alarm, and an excess CO<sub>2</sub> alarm. Preferably, these indicator, controls and alarms are duplicated on the exterior of the capsule. The activation of any of the alarms may be arranged to automatically depressurize the capsule and even to operate the actuator to release and 'pop' the canopy. A  
10 standby pressure vessel or electric battery may be needed to effect such functions despite a mains power failure.

#### DESCRIPTION OF EXAMPLES

Having portrayed the nature of the present invention, a particular example will  
15 now be described with reference to the accompanying drawings. However, those skilled in the art will appreciate that many variations and modifications can be made to the example, and many other examples can be devised, without departing from the scope of the invention as outlined above. In the accompanying drawings:

20 Figure 1 is a perspective view of the capsule of the chosen example with the canopy closed and a user seating inside.

Figure 2 is a perspective view of the capsule of Figure 1 with the canopy  
25 open and no user visible.

Figure 3 is a longitudinal cross-section of the closed capsule taken on  
plane III-III of Figure 1, the user not being shown.

30 Figure 4A is a perspective view of the underside of base and canopy frames with the canopy frame in the closed position, showing the manner in which the multiple latches are operated in unison.



Figure 4B is a side elevation of the base and canopy frames of Figure 4A with the canopy frame in a half open position.

5 Figure 4C is a side elevation of the base and canopy frames of Figures 4A and 4B with the canopy frame shown in the closed and latched position.

Figure 5A is an enlarged elevational detail of one of the latches of the capsule of Figure 1 in its closed or locked position, and showing portion of the latch operating mechanism.

10 Figure 5B is a sectional view of the latch and mechanism of Figure 5A taken on section line V – V of Figure 5A.

Figure 6A is an elevational detail of the latch and mechanism of Figure 5A shown in the open or unlatched position.

15 Figure 6B is a sectional view of the latch and mechanism of Figure 6B taken on section line VI – VI of Figure 6A.

20 Figure 7 is a sectional detail through the base and the actuator handle showing the manner in which the internal and external handles are connected.

25 Figure 8 is a sectional side elevation, taken on plane III-III of Figure 1, showing the arrangement of the air supply system, controls, alarms and auxiliary equipment suitable for use with the chosen example.

Figure 9A is a sectional detail of a safety interlock in the locked position and Figure 9B is the same view with the interlock in the unlocked position.

30 Figure 10A is a side elevation of the canopy and base frames in the open position showing a first alternative latching arrangement, while Figure 10B is a similar view to that of Figure 10A with the canopy and base frames in the closed position.

Figure 11A is a side elevation of the canopy and base frames in the closed position showing detail of a second alternative latching arrangement, while Figure 11B is a similar view to that of Figure 11A with the canopy and base frames in the open position.

Turning to Figures 1, 2 and 3, the basic components of the capsule 10 of the chosen example include a molded base 12, which includes an integrally-molded chair 14, and a curved downward and forwardly sloping canopy 16, which includes a large elongate and convex oval transparent window 18 and depending generally-planar triangular panels 20 on each side. Canopy 16 is curved both from side-to-side and from front-to-back and is pivotally attached at the lower front to the front of base 12 by a hinge assembly 22. A gas strut 24 on each side near hinge assembly 22 is designed to both take the weight of canopy and limit the rate at which it can be swung open or closed. In Figures 1 and 3, canopy 16 is shown closed, while in Figure 2, it is shown open. The outline of a person 26 seated on chair 14 is indicated in Figure 1, but not in Figures 2 and 3.

In this description it will be convenient to refer to the space enclosed by canopy 16 and base 12 as the hyperbaric chamber – since it can be pressurized – and to refer to the entire device as the capsule.

As best seen from Figure 2, base 12 has a generally horizontal bottom 28 with a curved front portion 30 and a generally upright back 32 with a curved top 34 portion. Bottom 28 (including curved front portion 30) defines a generally horizontal U-shape that has an upward-facing peripheral edge 36, while back 32 defines a generally vertical U-shape that has a forward-facing peripheral edge 38. The rear of bottom peripheral edge 36 joins the bottom of back peripheral edge 38 at an angle indicated at 40, which corresponds to the angle indicated at 42 of triangular side portions 20 of canopy 16.

While peripheries 36 and 38 could form a continuous peripheral seal-line against which a sealing strip fitted around the inside of canopy 16 could rest, in this example the continuous seal-line 44 is formed by the faces of shoulders 45a and

45b that up-stand from peripheral edges 36 and 38 (respectively). A flexible resilient seal-strip 47 (Figures 2 and 6A and 6B) is fitted around the entire internal periphery of the canopy so that it engages with base 12 inboard of canopy 16. The arrangement is such that, when canopy 16 with attached seal-strip 47 is lowered onto base 12 to the closed position (as in Figure 1), seal-strip 47 is brought to rest against shoulder 45a of bottom 28 of base 12 and against shoulder 45b of back 32 of base 12. Thus, internal pressure in capsule 10 will press seal-strip 47 downwards into sealing contact with bottom 28 and backwards into sealing contact with back 30. [This is shown and described in more detail with reference to Figures 6A and 6B.]

After being lowered to its closed position, canopy 16 can be secured to base 12 by pivoting side hook-like latches 50a – 50c on each side of base 12 to engage corresponding latch pins 52a – 52c each side of canopy 16. A pair of pivoting top hook-like latches 50d engage a common latch pin 52d (Figure 2) located inside the top rear of canopy 16. Latches 50a - 50d are mechanically linked (in a manner to be described) so as to operate in unison, latch 50c (Figures 1 and 2) being formed on the lower end of an external actuator or handle 54. Handle 54 is secured to a transverse shaft 84c (to be further described) that passes through back 30 of base 12 and is connected for conjoint operation with an internal handle 56. Thus, latches 50a - 50d can be operated in unison by person 26 seated in the capsule using handle 56 or by a person outside the capsule using handle 54.

The peripheral edges 36 and 38 of base 12 thus define a recess around base 12 within which the linear peripheral edges of triangular sides 20 of canopy 16 are located when the canopy is closed.

The window 18 of canopy 16 is joined to triangular side panels 20 by a curved fiber-reinforced plastic [FRP] skirt 60 molded onto and around the periphery of window 18, which is blown to shape in an oven without a mold from thick transparent plastic sheet material. Base 12, including the basic shape of chair 14, bottom 28, curved front 30, back 32 and its peripheral edges 36 and 38, is molded integrally from FRP. Included in this molding is a back support 62 and a seat support 64 (Figures 2 and 3) of chair 14 and a foot-well or floor 66 in front of chair

14. Chair 14 is completed by a back cushion 68 fitted on back support 62 and a seat cushion 70 fitted on seat support 64. The peripheral area of base 12 inboard of canopy 16 (when closed) is shaped so as to provide a peripheral land 44a against which seal strip 44 can rest and form a sealing engagement. Thus, closure of the canopy 16 onto the upper part of base 12 forms a hermetically sealed enclosure, except for the provision of inlet slots 72 for the pressurized air at the top of seat back support 62 and the provision of a pressure-regulating exhaust valve 74 between the wall of foot well 66 and curved front 30 of bottom 28 of base 12. A pair of wheels 76 is provided toward the rear of bottom 28 to assist movement of capsule 10 and a pair of adjustable feet 78 is provided near the front of bottom 28 to stabilize the capsule once it is in position (see Figure 3).

The latching mechanism will now be described in more detail with reference to Figures 4A – 5B, which illustrate the engaging peripheries of base 12 and canopy 16 with most other parts removed. The periphery of base 12 incorporates a metal frame 80 that carries hook-like latches 50a - 50d and half of hinge assembly 22. Similarly, the complementary periphery of canopy 16 incorporates a metal frame 82 that carries latch pins 52 and the other half of hinge assembly 22. Frames 80 and 82 are shown in the position for a closed canopy in the Figures 4A & 4C and in the position for a half-open canopy in Figure 4B.

Hook-like latches 50a – 50c are arranged in opposed pairs, one latch of each pair (eg, 50a) being located opposite the other on each side of the base frame, the latches of each pair being fixed to respective ends of a common transverse shaft. Thus, latches 50a are mounted on each end of shaft 84a, latches 50b are mounted on each end of shaft 84b and latches 50c are mounted on each end of shaft 84c. Short bell-cranks 86a, 86b and 86c are fixed to the centers of shafts or rods 84a, 84b and 84c (respectively), the free end of crank 86a on shaft 84a being pivotally attached to a horizontal actuator rod 88. The free ends of cranks 86b and 86c on shafts 84b and 84c are pivotally attached to a common generally vertical actuator rod 90 behind the back of the chair (not shown). Rear end of rod 88 is pivotally linked to lower end of rod 90 by a bell-crank 92 that is mounted for rotational movement about a fixed transverse tie-rod 93, which – together with similar tie rods 94 and 95 – serve to tie sides of frame 80 together. Upper

extremity of actuator rod 90 is coupled to latches 50d by a push-rod 96. This arrangement ensures that all latches 50a - 50d will operate in unison when motivated by handle 54 or 56, both of which are attached to shaft 84c. Internal handle 56 is secured to shaft 84c within a seal-tube tube 98 (Figure 4A) that  
5 prevents air leakage along that handle from within the hyperbaric chamber.

The operation of hook-like latch 50a shown in Figure 1 is illustrated in the detail views of Figures 5A – 6B. As in Figure 1, latch 50a is shown in Figures 5A and 5B engaged with latch pin 52a so that triangular side portion 20 of canopy 16 is  
10 locked to bottom portion 28 of base 12. It will be seen from Figure 5A that the throat 53 of latch 50a slopes upwards toward latch pin 52a; that is, it has a re-entrant form such that, when upward force is applied to pin 52a, latch 50a tends to close further rather than open. As described with reference to Figures 4A – 4C, latch 50a is fixed to one end of transverse shaft 84a that can be rotated by bell-  
15 crank 86a and actuator rod 88 to engage or disengage latch 50a with its pin 52a, rod 88 being pivotally attached to bell-crank 86a by pin 87. Canopy frame 82 is encased within a molded FRP wall 20a that has a foam core 20b. Similarly, frame member 80 of the bottom 28 of base 12 is encased in an FRP molding 28a, a bearing sleeve 99 being inserted into molding 28a and frame member 80 to carry  
20 shaft 84a.

Molding 28a forms the peripheral shoulder 45a on base portion 28 that, in turn, forms upwardly facing seal-line or surface 44. As shown in Figure 5B, a sealing strip 100 (shown here in section) is glued to the inside of canopy side 20 near its  
25 bottom and has a flap 101 that rests on seal-line 44 of base portion 28. Under hyperbaric pressure within the chamber, flap is pressed onto seal-line 44 to hermetically seal the chamber. A cushion 103 is glued to the bottom edge of canopy side 20 to cushion the contact between that portion of canopy 16 and base 12 upon lowering of the canopy, cushion 103 not being intended to function  
30 as a seal.

It will be noted that the planar triangle-shaped canopy sides 20 will flex outwards toward latches 50a when the capsule is under pressure, stretching seal 100, until sides 20 contact latches 50a. The force thus applied to latches 50a will be

transferred to transverse shaft 84a, which can readily be designed to carry such forces, being in tension. The same considerations apply to pairs of latches 50b and 50c, which are carried by shafts 84b and 84c, as described with respect to Figures 4A – 4C, above.

5

Figures 6A and 6B are similar views to Figures 5A and 5B respectively and show side 20 of canopy 16 slightly raised from bottom 28 of base 12. In Figures 6A and 6B latch 50a is shown in the open position, having been moved by a pushing force applied to rod 88 that rotates bell-crank 86a, shaft 84a and hook-like latch 50a in the clockwise direction.

10

Figure 7 is a sectional view illustrating one way in which the internal and external actuator handles 56 and 54 may be arranged on the common shaft 84c in a manner that maintains the desired hermetic seal of canopy-to-base of the capsule. An open-ended bearing tube 98 is molded into the side of back 32 of base 12 to house shaft 84c, the inner end of tube 98 being fitted with a C-clip 104. The central periphery of tube 98 is slotted at 105 to accommodate handle 56 and allow the handle to be moved through a sufficient angle to permit operation of latches 50a - 50d. With shaft 84c in place (ie, passing through) tube 98, an inner bearing 106 for shaft 84c is pushed into tube 98 from its external end along shaft 84c until it abuts C-clip 104, bearing 106 being fitted with a pair of inner O-rings 108 to sealingly engage shaft 84c and an outer pair of O-rings 110 to engage the bore of tube 98. Next, a hub 112 is pushed along shaft 84c into tube 104 until it abuts bearing 106, hub 112 being cross-drilled and threaded to take a corresponding screw-thread 56a formed on the lower end of handle 56. Hub 112 has an O-ring 114 on each side of handle 56 to engage the bore of tube 104. An outer bearing 116 that is substantially the same as inner bearing 106 (including inner an outer O-rings) is then pushed into tube 104 along shaft 84c and the two bearings and hub are held in place by an outer C-clip 118. Finally, outer handle 54 is fitted to the outer end of shaft 84c by cross-pin 119 and inner handle 56 is screwed into hub 106 and into a depression formed in shaft 84c to ensure that handle 56 can rotate shaft 84c. It will be seen that, while shaft 84c is located outside the pressurized portion of capsule 10 and handle 56 is located inside, air cannot escape past the handle 56 out of tube 104 or along shaft 84c.

15

20

25

30

The pressurization, control and monitoring of the capsule of this example will now be described. In this example independent control and monitoring of the pressure, oxygen concentration (and/or CO<sub>2</sub> concentration), humidity and temperature of air in the capsule is provided. The need to be able to set the desired pressure in a hyperbaric chamber is, of course, obvious. However, the need to monitor for temperature, CO<sub>2</sub> and humidity is dictated by the fact that these variables can quickly rise to uncomfortable – even dangerous – levels in a capsule of small volume like that of the chosen example. If supplemental oxygenation is not used, oxygen monitoring is desirable to (i) ensure that the oxygen concentration of air in the capsule does not fall significantly below that of the atmosphere and (ii) to generate an alarm in the event of an excessive rise. When supplemental oxygenation is used, it may be via a mask or via oxygen injection into the pressurizing air. In that case, it is desirable to have a separate indicator of mask oxygen concentration, and the readings of CO<sub>2</sub> or oxygen concentration in the capsule air may then be of little significance. Control of pressure, temperature and humidity can be achieved by known air-conditioning techniques and apparatus, except for the need for an air pump or blower of higher than normal pressure.

Figure 8 illustrates the basic arrangement of indicators and controls for the chosen example. An external set of indicators and controls is shown at 120 on the side of upright back 32 of base 12 of capsule 10. Internally, a set of indicators (comprising meters and alarms) is mounted in box 122 located at the bottom front of canopy 16 so as to face a seated user. A set of controls 124 is mounted on the inside of one of canopy panels 20 so as to be convenient for operation by the user. The internal indicators and controls 122 and 124 can duplicate the external indicators and controls 120. Cooled air is supplied to the interior of capsule 10 via a pipe 126 from an air-conditioning and pump unit 128 located at the bottom of the rear of base 12. Ideally, unit 128 can be controlled to vary air flow, relative humidity and temperature. The air inlet into the chamber comprises slots 72 (see also Figure 3) located above the back of chair 14. As already noted, air from the hyperbaric chamber is exhausted in a controlled manner through throttle valve 74 and exhaust outlet 130. Pressure regulation is achieved by varying the relative rate at which air flows into and out of the chamber. This may be done by the use

of a fixed air outflow rate and a variable air supply rate, a fixed inflow rate and a variable outflow rate, or by a combination of these methods. A controller unit 134, which accepts inputs from the sensors of monitoring unit 122 and user controls 124, is shown located under the seat of chair 14. Figure 8 also shows an oxygen  
5 bottle 136 located in the back 32 of base 12, though no connections are shown to it. Oxygen from this bottle may be used to inject supplemental oxygen into to the input air in pipe 126 or it may be used to provide oxygen to a mask (not shown).

If desired, provision may be made for automatic depressurization and latch  
10 release in the event of power failure or excessive chamber air temperature, humidity or CO<sub>2</sub> concentration. Excessive CO<sub>2</sub> concentration and/or temperature can arise where air flow is too low due to malfunction or power failure and may not be noticed by the user in time to take remedial action. In this example, this safety feature is provided by:

- 15 (i) ensuring that power failure or the operation of the CO<sub>2</sub> alarm will deactivate air-conditioning and pump unit 128 and open inlet pipe 126 to atmosphere,
- (ii) fully open exhaust valve 74, if it is controllable (air will still exhaust from the chamber if valve is not controllable), and
- 20 (iii) operate an automatic latch actuator unit 140 that is located in back 32 of base 12 and connected to shaft 84c.

Thus, as soon as the pressure within capsule 10 is equilibrated with atmospheric, the latches will be opened and struts 24 will pop the canopy open enough to  
25 ensure circulation of ambient air through the chamber.

Desirably, the CO<sub>2</sub> sensor, controller 134 and automatic actuator 140 should have sufficient standby battery power to operate in the event of power failure. However, the power requirement of actuator 140 may be too large for the standby battery  
30 suited to the sensors and controller, so spring, pneumatic or other energy storage means can be used to power unit 140.

A further safety feature envisaged in a modified form of the chosen example is a pressure operated interlock that will prevent the canopy from being opened



prematurely by the user. This may result in forceful and dangerous opening of the canopy if the user has sufficient strength to force internal handle 56 and release latches 50a - 50d. A suitable safety interlock, located in canopy frame 82, is shown in Figures 9A and 9B, which illustrate a modified form of canopy and base.

5 The interlock comprises a diaphragm 142 mounted in canopy frame 82, the diaphragm carrying a slide-bolt 144 for movement outwards to engage a slot 145 in a catch-plate 146 that is fixed to base frame 80. A spring 148 biases bolt 144 away from catch-plate 146 so that, if the chamber pressure approximates ambient air pressure, the capsule can be opened normally and without the need to touch

10 bolt 144. On the other hand, if the chamber pressure is significantly higher than ambient, and if handle 56 is forced to prematurely open latches 50a - 50d, the interaction of bolt 144 and slot 145 in catch-plate 146 will prevent the canopy from opening more than enough to ensure immediate pressure equalization. To fully open the canopy after operation of the latches in this way, where bolt 144 is still

15 extended because of a fault, the user can manually withdraw bolt 144. There will be little resistance to this since the chamber is under no pressure.

The modified canopy side 20 and base bottom 28 shown in Figures 9A and 9B, illustrates another way in which the side forces of canopy sides 20 can be

20 restrained. This is through the side plates 146 that can be placed at intervals around the periphery of the base, as needed, though more than one interlock bolt will not be normally be needed. It will also be seen that the manner in which the seal-line or surface 44 is formed can be varied as desired. Different forms of seal-strip may also be used, though that illustrated is of the same section as strip 100

25 shown in Figures 5B and 6B (and it has been referenced accordingly).

Other variations of the latching mechanism may also be employed. Some of these are shown in Figures 10A – 11B. In the variant of Figure 10, each side of canopy frame 82 carries two sliding notched latch plates 150a and 150b that engage

30 respective rows of latch pins 152a and 152b located on each side of base frame 80. The sliding plates 150a are on the bottom edge of canopy 82 and are moved backwards and forwards by an actuator lever 154 and are coupled (by means not shown) to upper sliding plates 150b so that all plates move in unison to engage

and disengage latch pins 152a and 152b. Figure 10A shows the frames in the open position and Figure 10B shows the frames in the closed position.

The second variant, shown in Figures 11 and 11B, has mushroom-headed latch pins 160 depending from the bottom of canopy frame 82 that pass and project through holes 162 in base frame 80. Each latch pin 160 can be engaged by an open ended slot 163 in a locking plate 164 to prevent its withdrawal through hole 162. Locking plate 164 is fixed by bolts 165 to a carrier plate 166 that can be reciprocated with respect to base frame 80 by a rack and pinion mechanism 168 that is operated by an actuator lever 170. Figure 11A shows canopy frame 82 removed a little way from the base frame with latch plate 164 in the open or release position. Figure 11B shows latch pin 160 engaged by slot 163 when the canopy (not shown) is in the closed position and latch plate 164 is in the locked position.

**CLAIMS**

1 A hyperbaric capsule wherein:

an elongate base molding forms a forward-facing chair for a user, the chair having a seat and a back rising from the seat,

5 said base molding has a front portion that extends forward of the chair seat at user foot level,

said base molding has a rear portion that extends upwardly above the back of the chair and above user head level,

10 said base molding defines a peripheral seal-line that extends around said front portion, along each side of the chair and around said rear portion,

an elongate canopy extends forward and downward from above user head level at said back portion of the base to said front portion of the base,

an elongate transparent window is formed in said canopy,

15 the canopy is moveable between an open position, where a user can freely move to the chair from the side of the capsule, and a closed position where a seated user is fully enclosed by the base and the canopy, and

said canopy defines a peripheral seal-line that is adapted to engage with said base seal-line to form an air-tight seal between the canopy and the base when the canopy is in the closed position.

20

2 A hyperbaric capsule according to claim 1 wherein:

said canopy has a convex external surface that is curved both front-to-back and side-to-side,

25 said window also has a convex outer external surface that is curved both front-to-back and side-to-side, and

said window extends at least from user head level to the level of the seat of the chair, when the canopy is closed.

3 A hyperbaric capsule according to claim 1 or 2, having:

30 latching means operable from both within and outside the capsule for securing the canopy to the base when the canopy is in the closed position to permit pressurization of the capsule, and for releasing the canopy from the base for movement to the open position.

4 A hyperbaric capsule according to claim 3 wherein said latching means includes:

a plurality of latches spaced around said peripheral seal-line of the base,  
a plurality of latch pins spaced around said peripheral seal-line of the  
5 canopy for engagement by respective ones of said latches,  
inside actuator means operable from inside the capsule when the canopy is  
in the closed position to secure and release all said latches in unison, and  
outside actuator means operable from outside the capsule when the  
canopy is in the closed position to secure and release all said latches in unison.

10

5 A hyperbaric capsule according to claim 4 wherein:

said latches include hook members moveable between a secure position in  
which said hook members engage respective ones of said latch pins when the  
canopy is in the closed position and a release position in which said members  
15 disengage said respective ones of said latch pins, and

said hook members have an over-center action whereby an opening force  
applied to the canopy, when said hook members are in said secure position, acts  
to bias said hook members toward the secure position, thereby inhibiting  
operation of said inside and outside actuator means when the capsule is under  
20 pressure.

6 A hyperbaric capsule according to claim 5 wherein:

the base has a first U-shape periphery which is generally horizontal and  
which defines a first portion of said base seal-line,

25 said first U-shape periphery extends from below the seat on each side of  
the chair and around said front portion of the base,

the base has a second U-shape periphery which is generally vertical and  
which defines a second portion of said base seal-line,

said second U-shape periphery is in the form of an inverted U that extends  
30 from below the seat on each side of the chair and over the back of the chair,

said first U-shape periphery and said second U-shape periphery join at a  
given angle below the seat, completing said base seal-line,

the canopy includes two opposed downwardly extending side portions of  
generally triangular form,

each side portion of the canopy forms a canopy angle that is substantially equal to said given angle, each side portion also defining portion of said canopy seal-line, and

the side portions of the canopy fit into said join of the first and second U-shape peripheries on each side of the capsule when the canopy is in the closed position.

7 A hyperbaric capsule according to claim 6 wherein:

said hook members are located externally of the base on each side thereof near the chair and near said join,

respective ones of said latch pins are located on and externally of said side portions of the canopy and are arranged for engagement by said externally located hook members.

15 8 A hyperbaric capsule according to claim 7 wherein:

said externally located hook members are arranged in opposed pairs,

the hook members of each of said pairs are fixed to respective ends of a common substantially horizontal shaft that extends transversely through the base molding, the hook members of each pair being movable by rotation of their respective shaft to engage and release their respective latch pins on the side portions of the canopy,

outward movement of the side portions of the canopy under pressure is resisted by abutment of the side portions with the hook members of a pair and tension within their respective shaft.

25

9 A hyperbaric capsule according to any one of claims 6 – 8, wherein,

the canopy is hingedly attached to the base so that, when the canopy is in the closed position, at least part of the side portions of the canopy lies inwards of said first and second U-shaped peripheries of the base on each side of the capsule, whereby outward movement of said side portions of the canopy under pressure is resisted by said first and second U-shaped peripheries of the base.

30

10 A hyperbaric capsule according to any preceding claim wherein:

the canopy is hingedly attached to the front portion of the base for movement about a transverse horizontal axis, and

gas struts are fitted between the canopy and the base on each side of the front portion of the base to counterbalance the weight of the canopy when open or  
5 when being opened.

11 A hyperbaric capsule according to any preceding claim wherein:  
a pressure-operated lock is provided to prevent the opening of the canopy while there is super-atmospheric pressure within the capsule.

10

12 A hyperbaric capsule according to any preceding claim having:  
means adapted to supply cooled air under pressure to the interior of the capsule, and

control means within the capsule adapted to indicate and/or regulate the  
15 temperature of the air supplied to the capsule.

13 A hyperbaric capsule according to any preceding claim having:  
means adapted to monitor the CO<sub>2</sub> concentration of air within the capsule,  
and

20 alarm means connected to said monitoring means adapted to signal the user when a predetermined concentration of CO<sub>2</sub> is reached.

14 A hyperbaric capsule according to claim 13 having:  
emergency release means operable to effect automatic depressurization of  
25 the capsule and release of said latching means when said predetermined concentration of CO<sub>2</sub> is reached.

15 A hyperbaric chamber according to any preceding claim having:  
oxygen supply means adapted to supply oxygen gas at hyperbaric  
30 pressure to a user within the capsule, said oxygen supply means including a face mask by which oxygen enriched air can be supplied to a user seated and enclosed within the capsule.

16 A hyperbaric chamber according to any preceding claim, wherein:

the width of the capsule is less than that of a standard door frame, and the base is fitted with wheels or rollers by which the capsule can be moved to or transported within a domestic location.

- 5    17    A hyperbaric capsule including:  
a base molding that includes an integrally molded chair for a user,  
a removable canopy adapted to fit over a user seated on the chair and to fit  
on the base around the chair and the user in a substantially air-tight manner, thus  
forming a chamber housing the seated user,  
10        latching means operable from both within and outside the capsule for  
securing the canopy to the base at a plurality of points about its periphery, and  
air supply means for supplying air under pressure to  
the chamber to generate hyperbaric pressure therein.

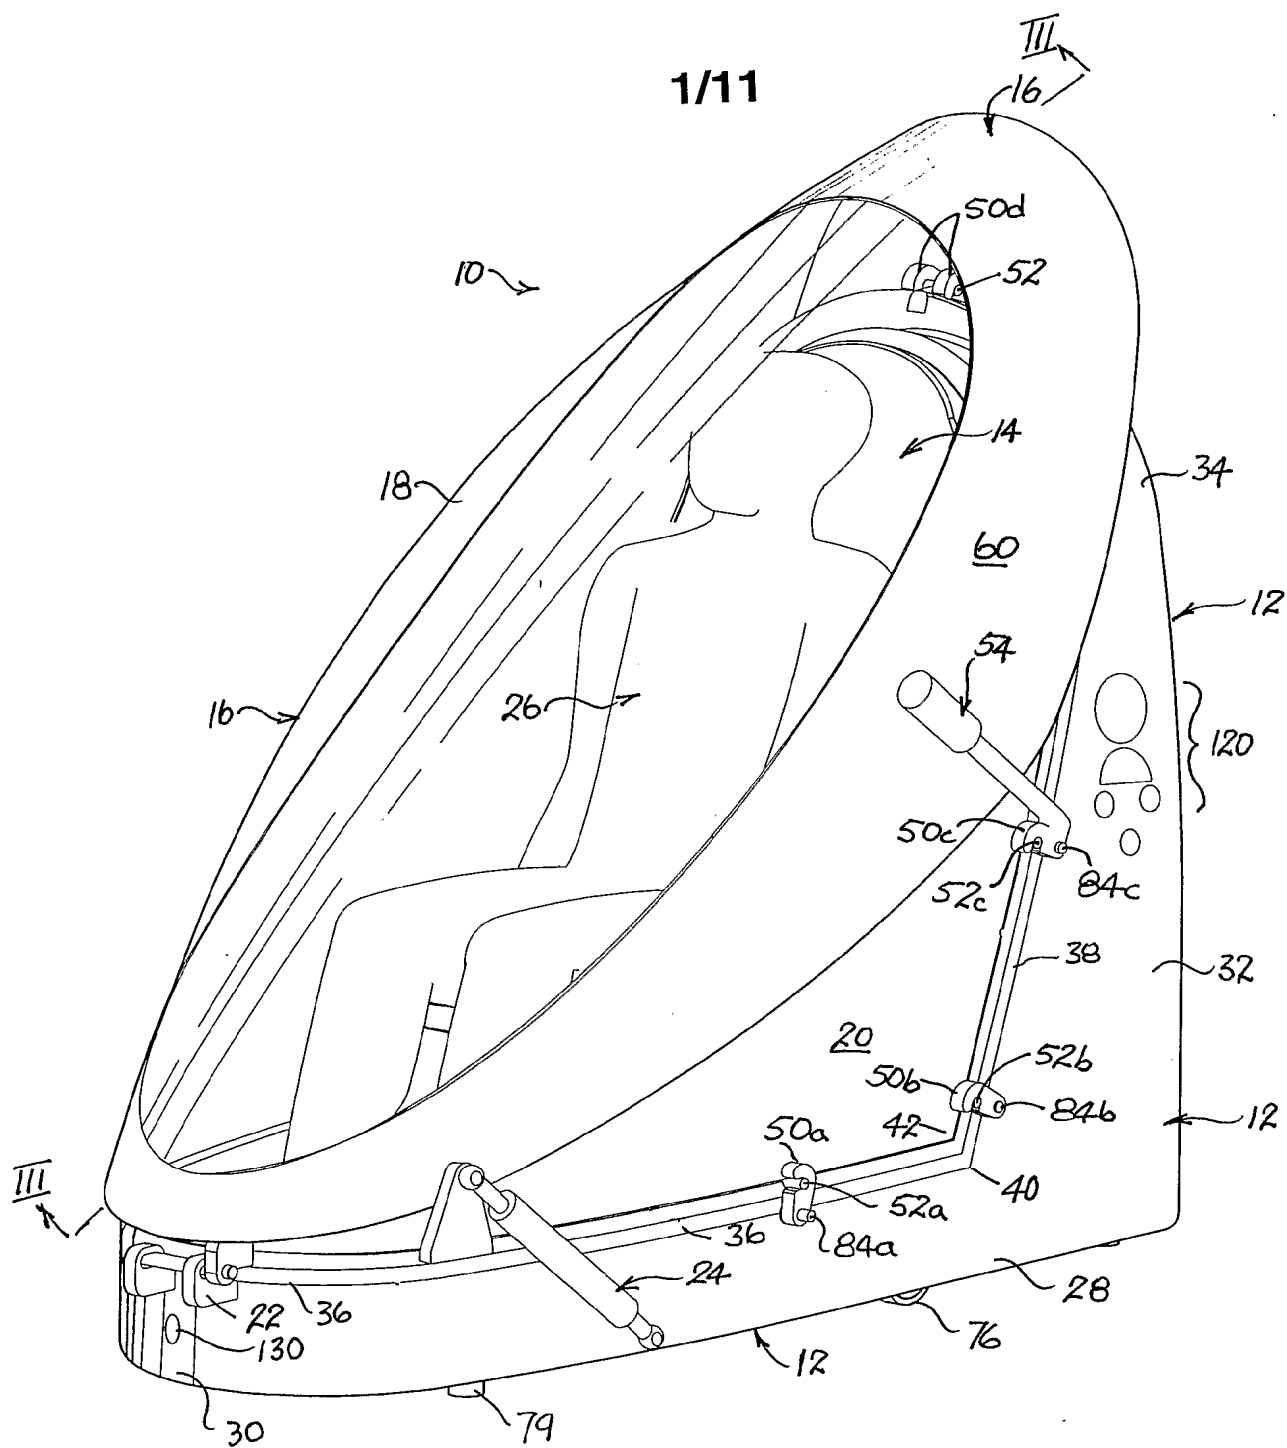


Fig.1



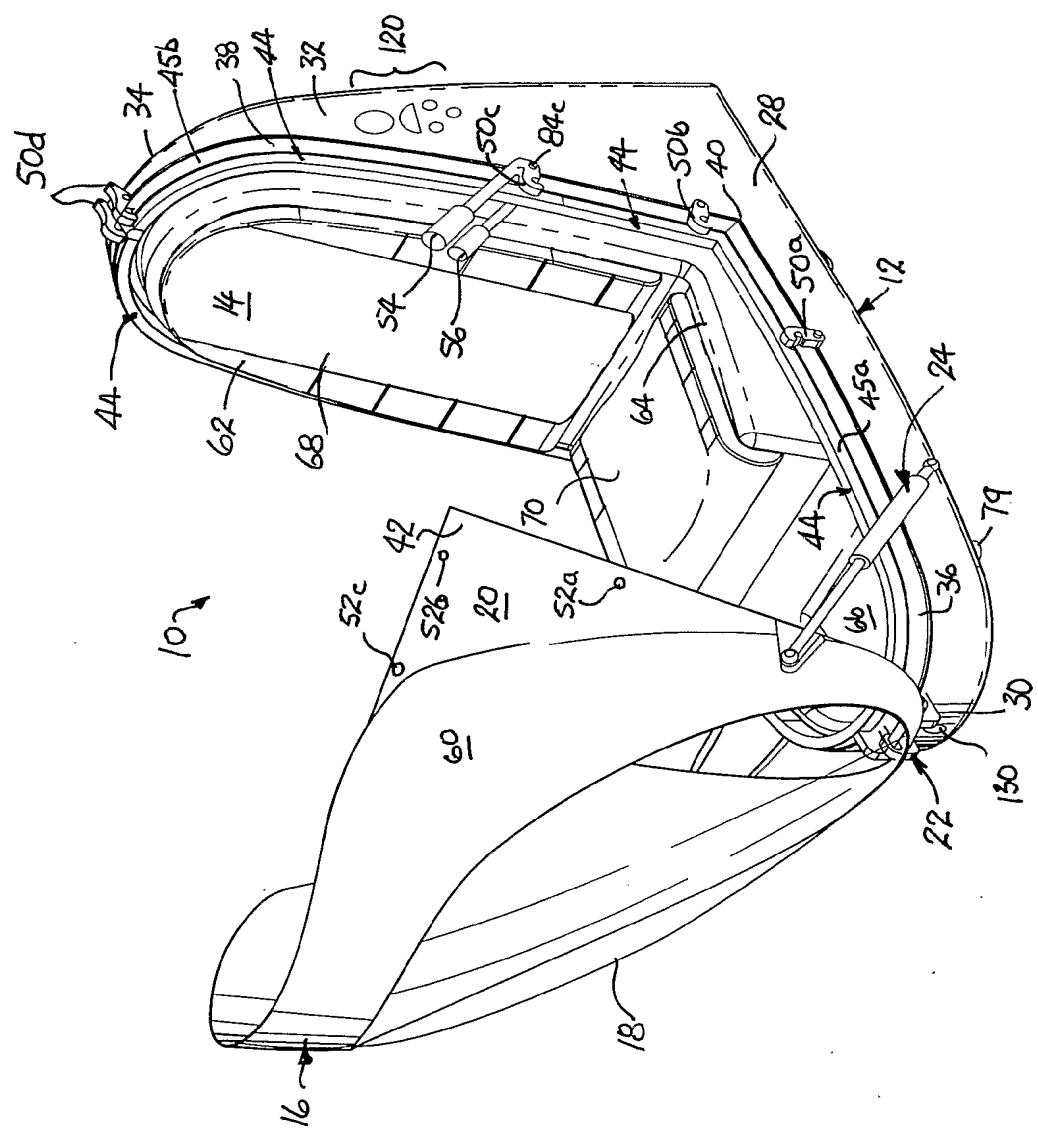


Fig.2

**3/11**



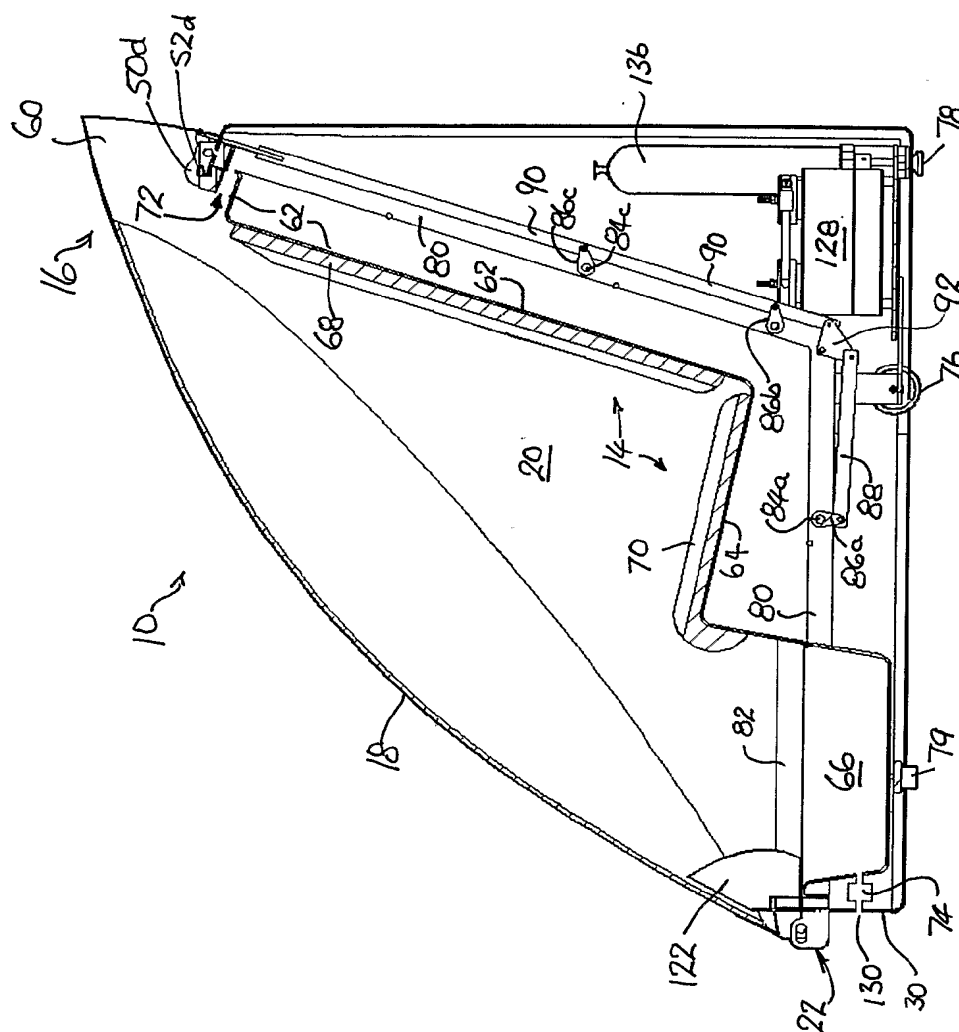


Fig. 3


4/11

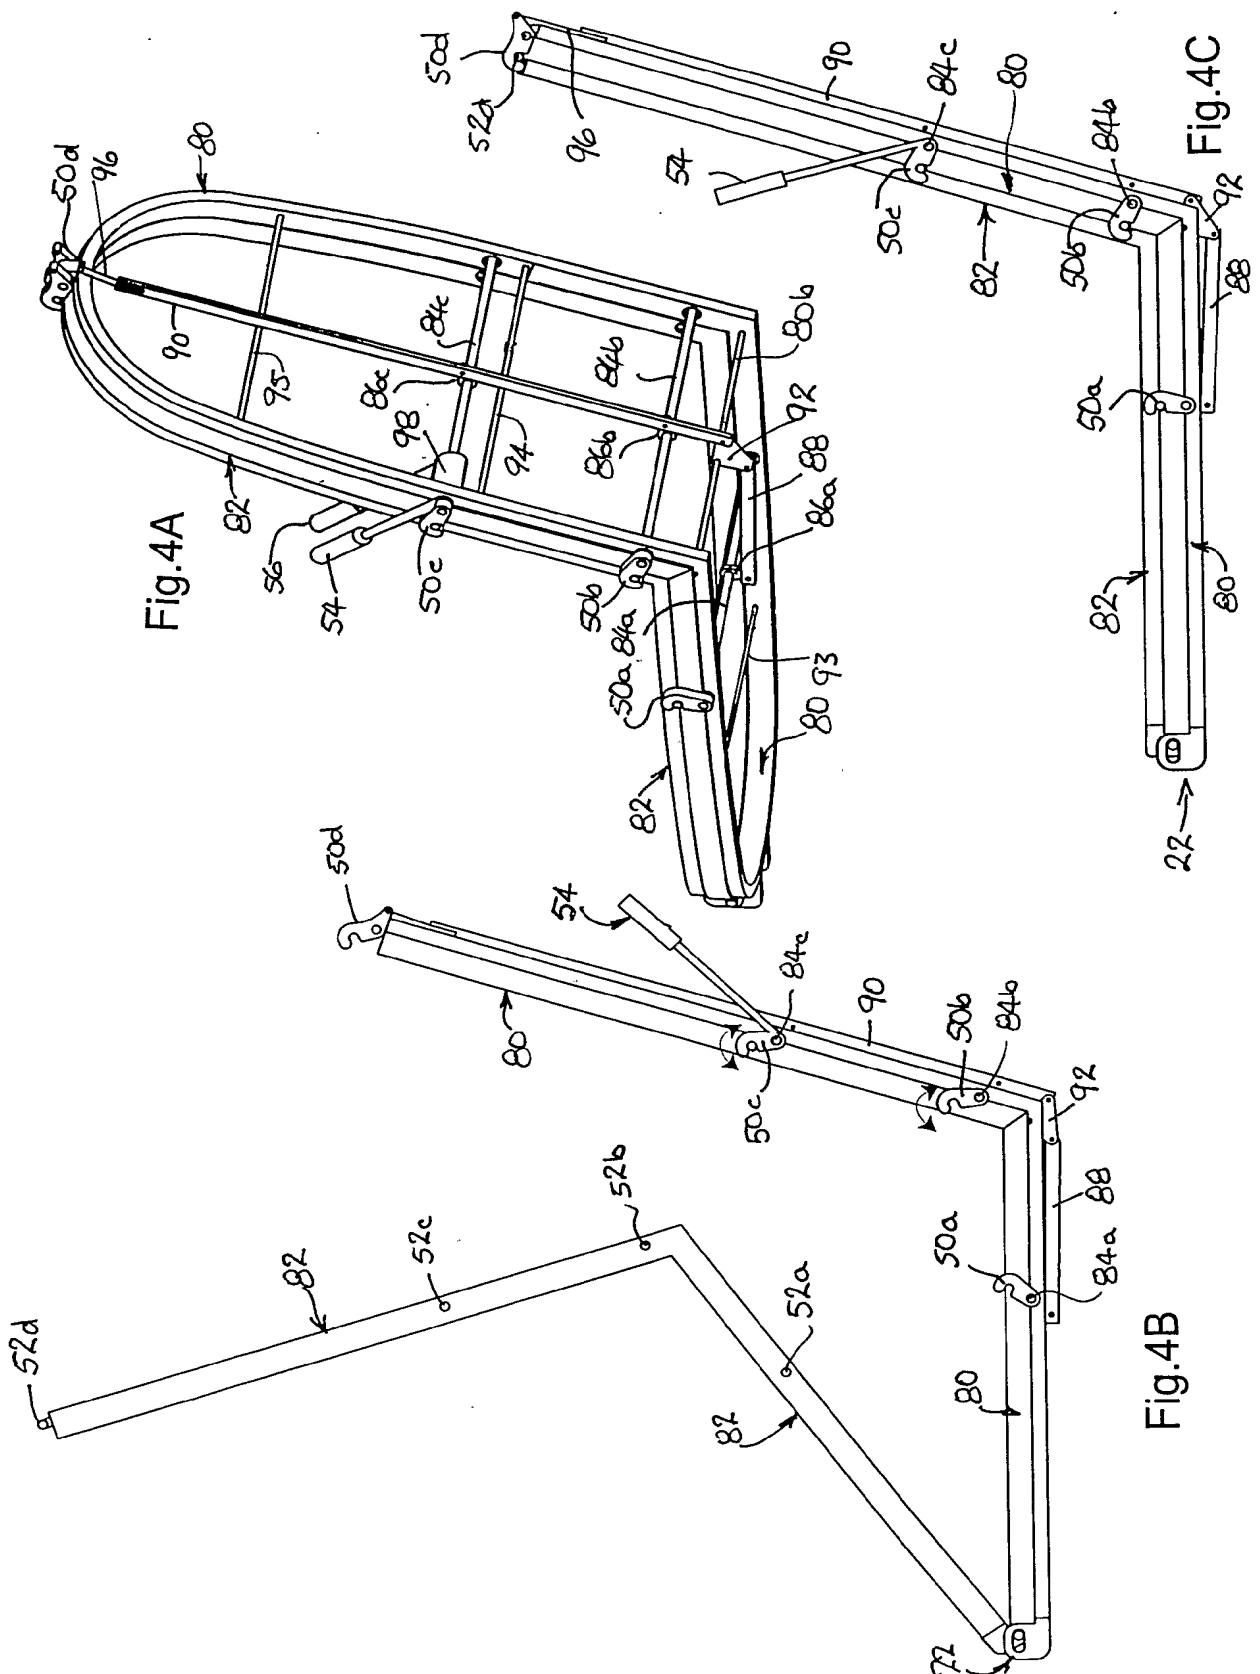



**5/11**

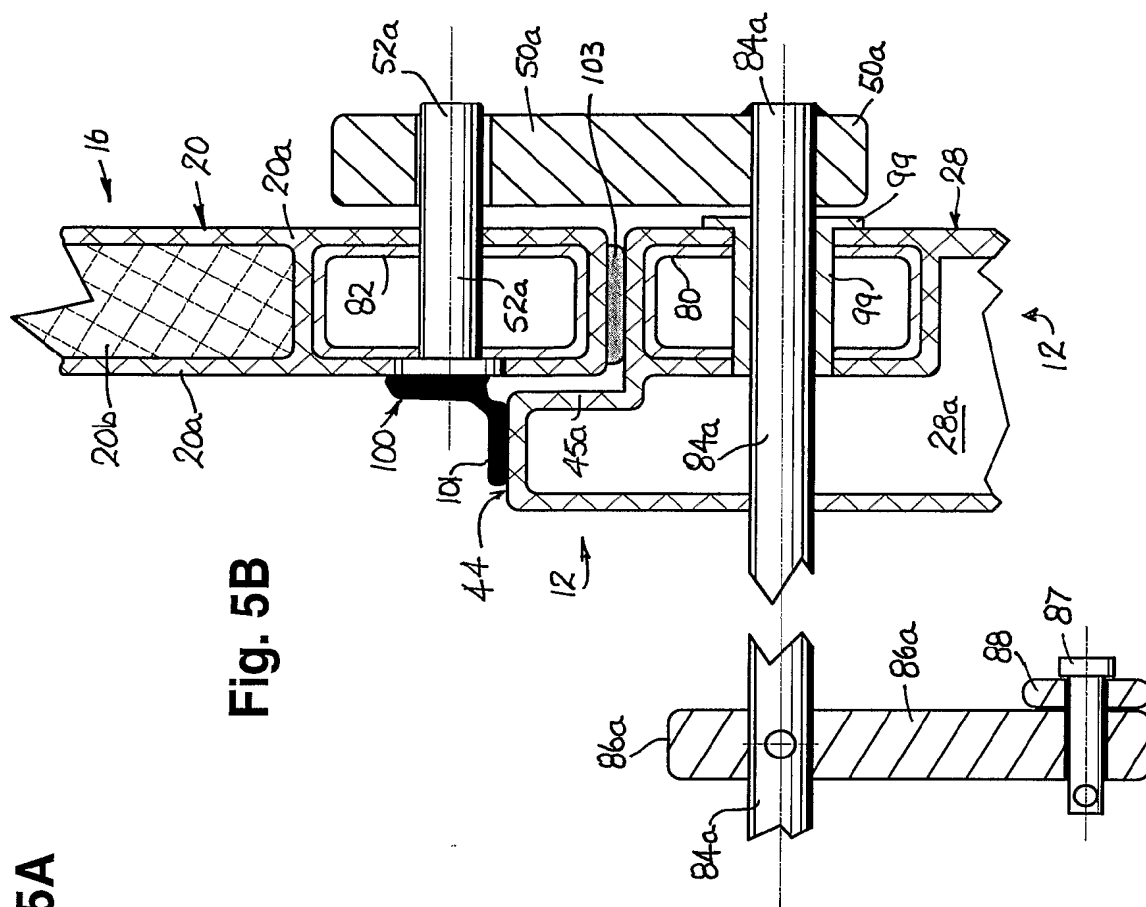

**Fig. 5B**

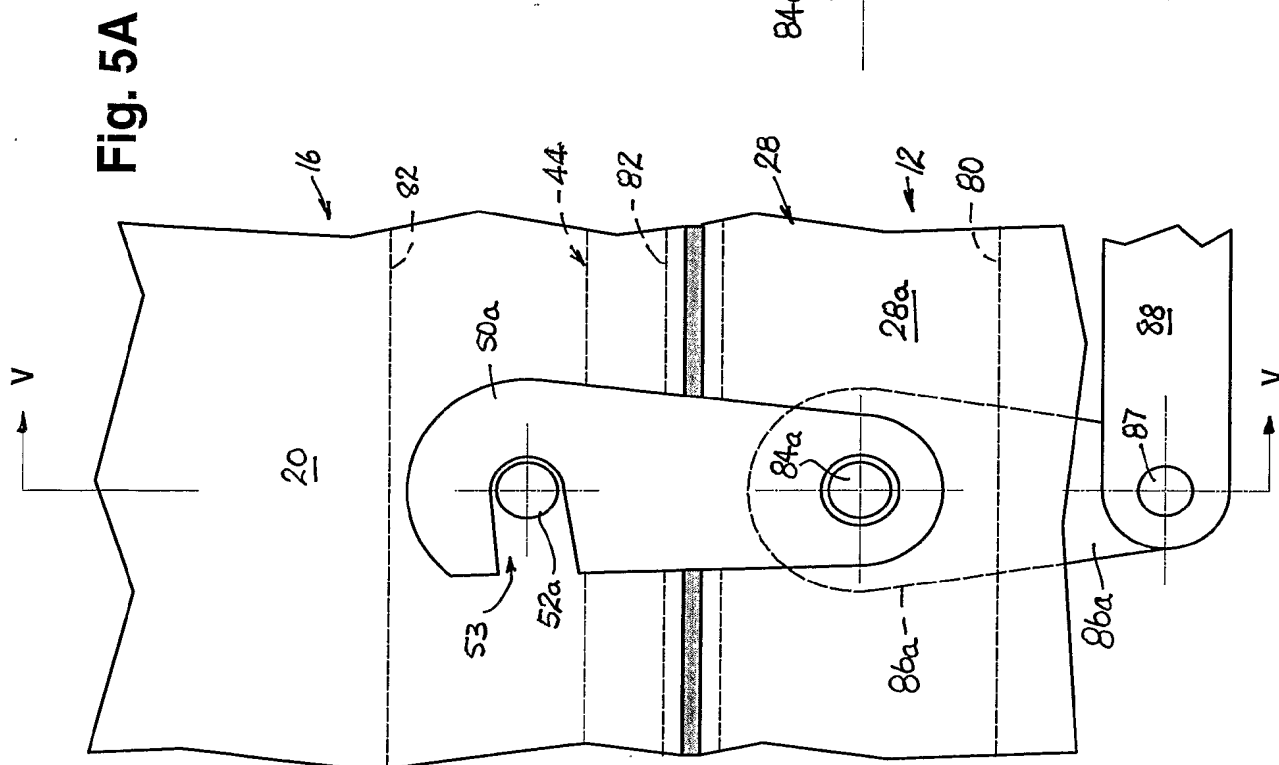

**Fig. 5A**

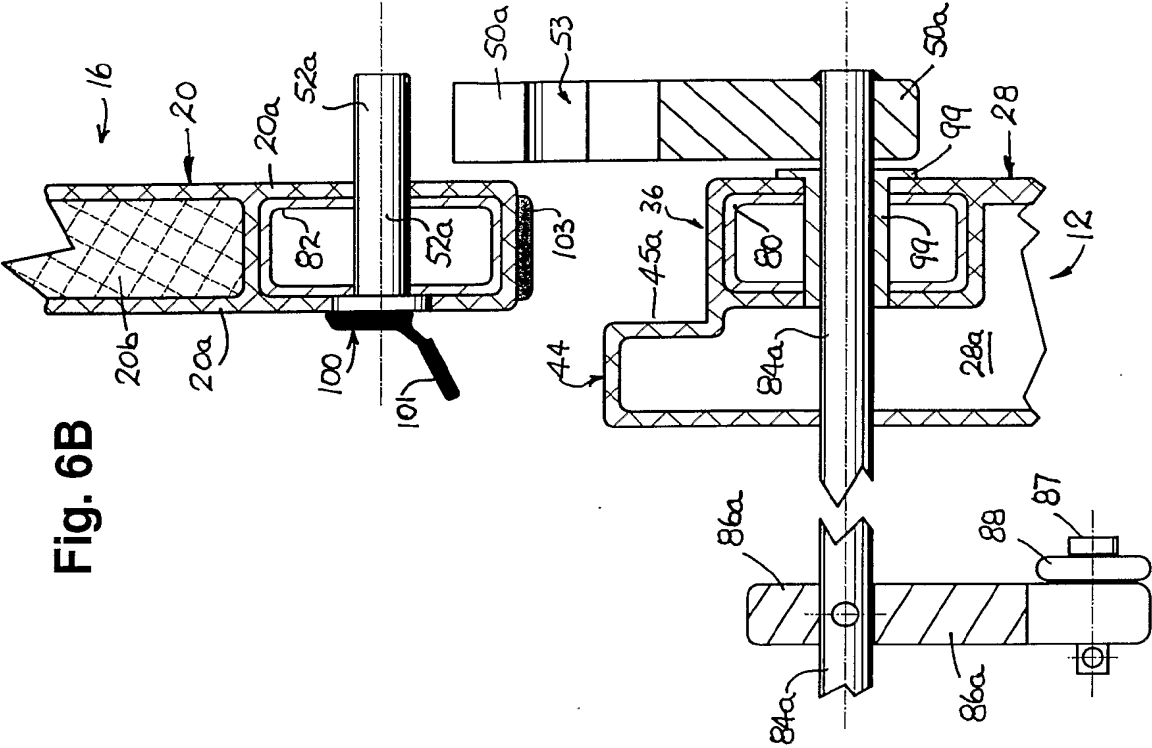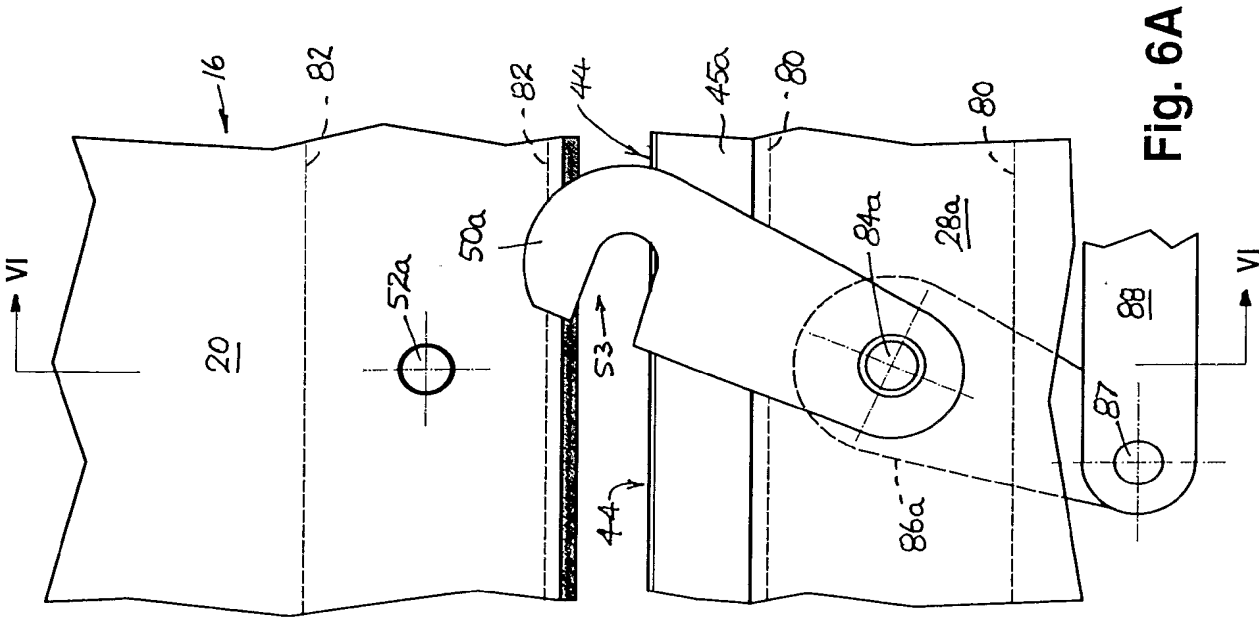



**8/11**

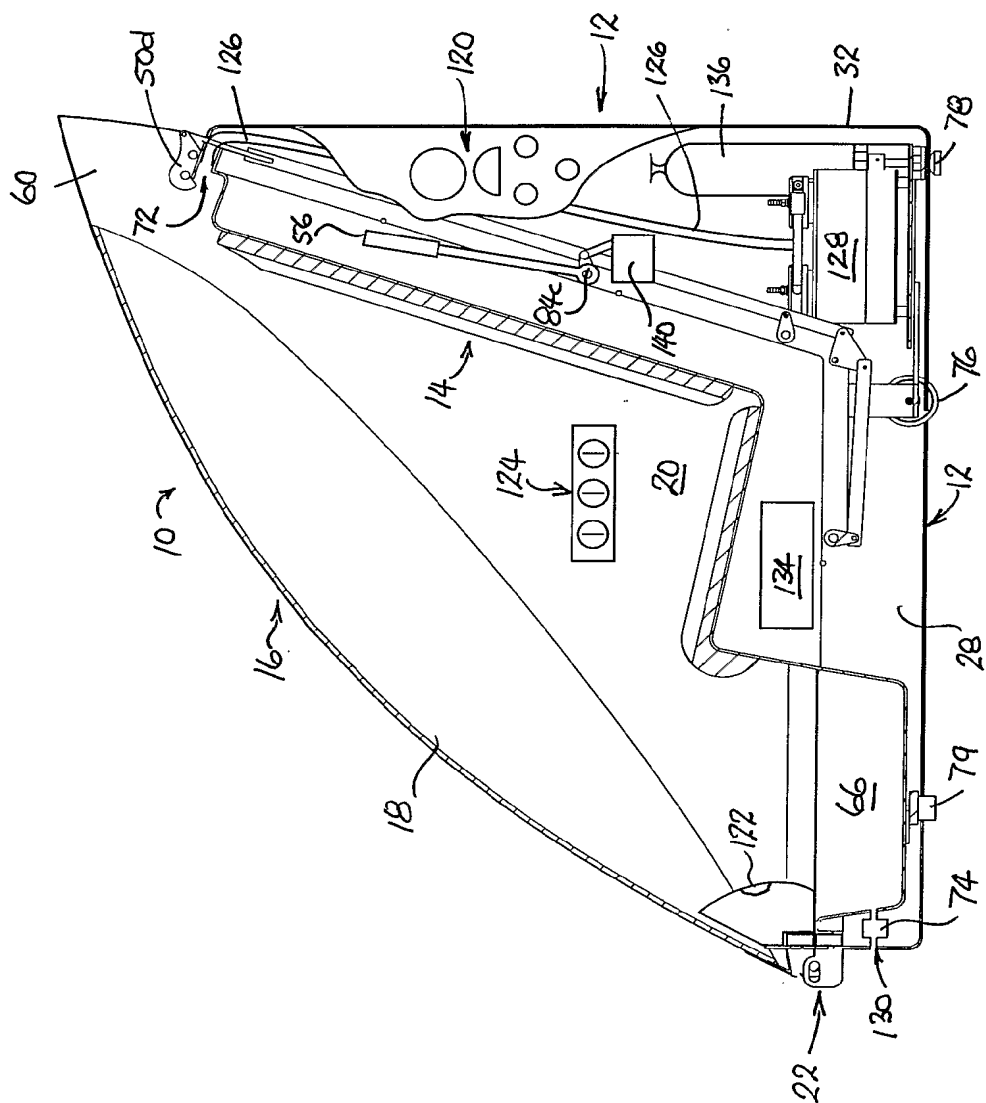


Fig. 8

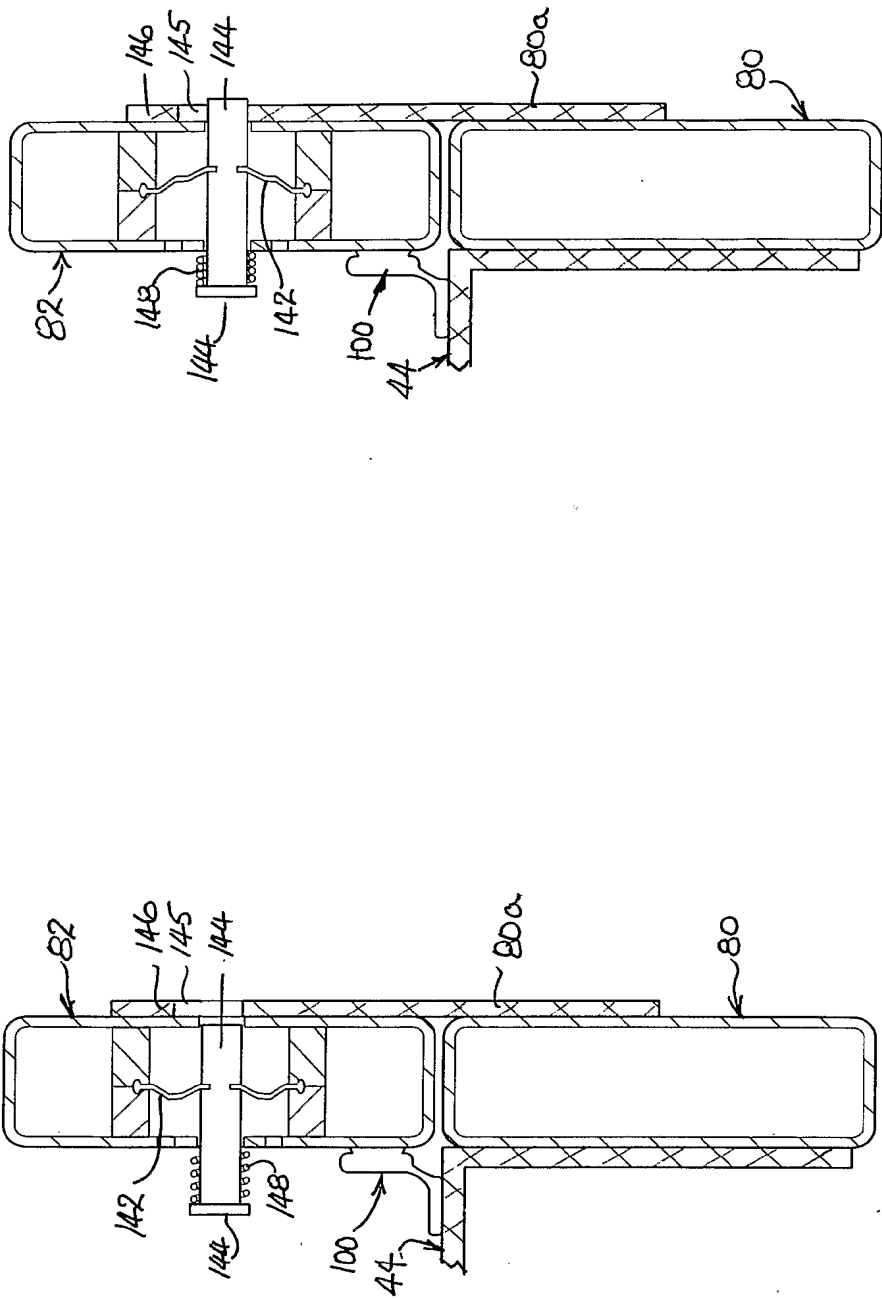


Fig.9B

Fig.9A



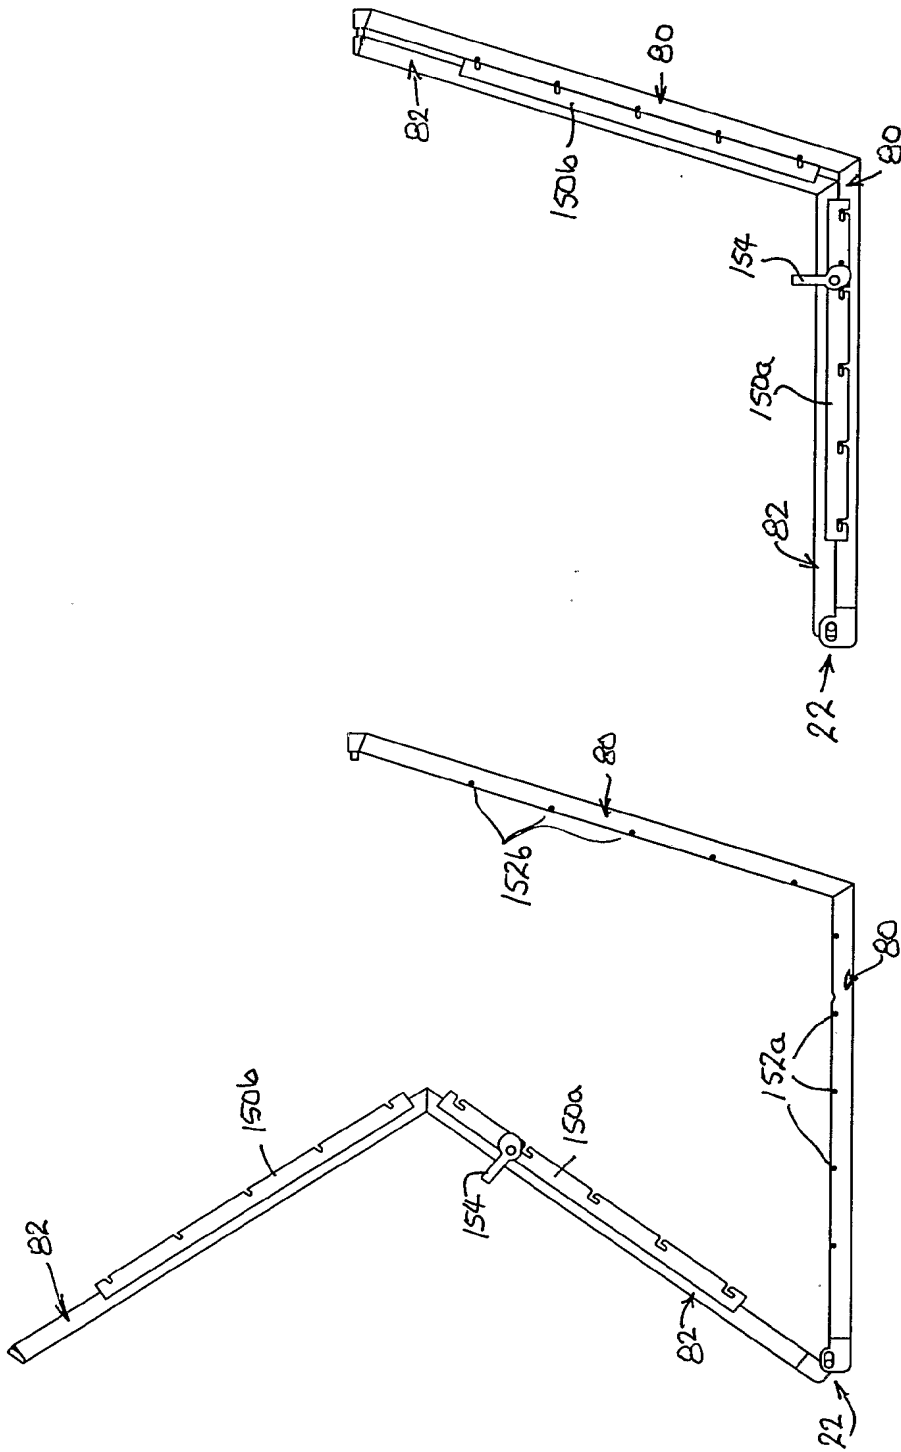


Fig.10B

Fig.10A

11/11

Fig.11B


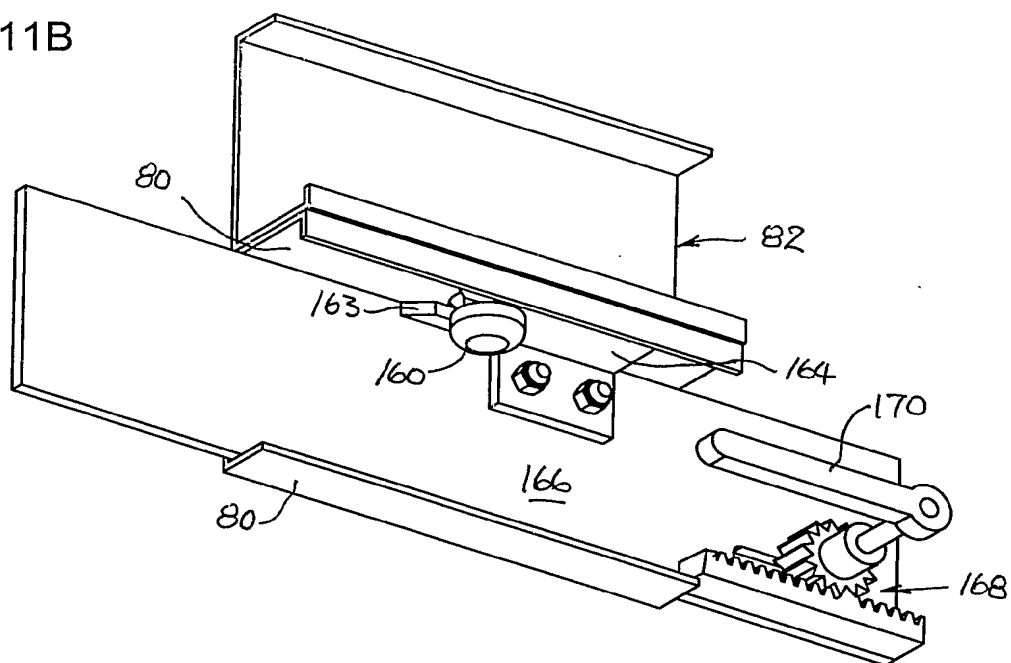


Fig.11A

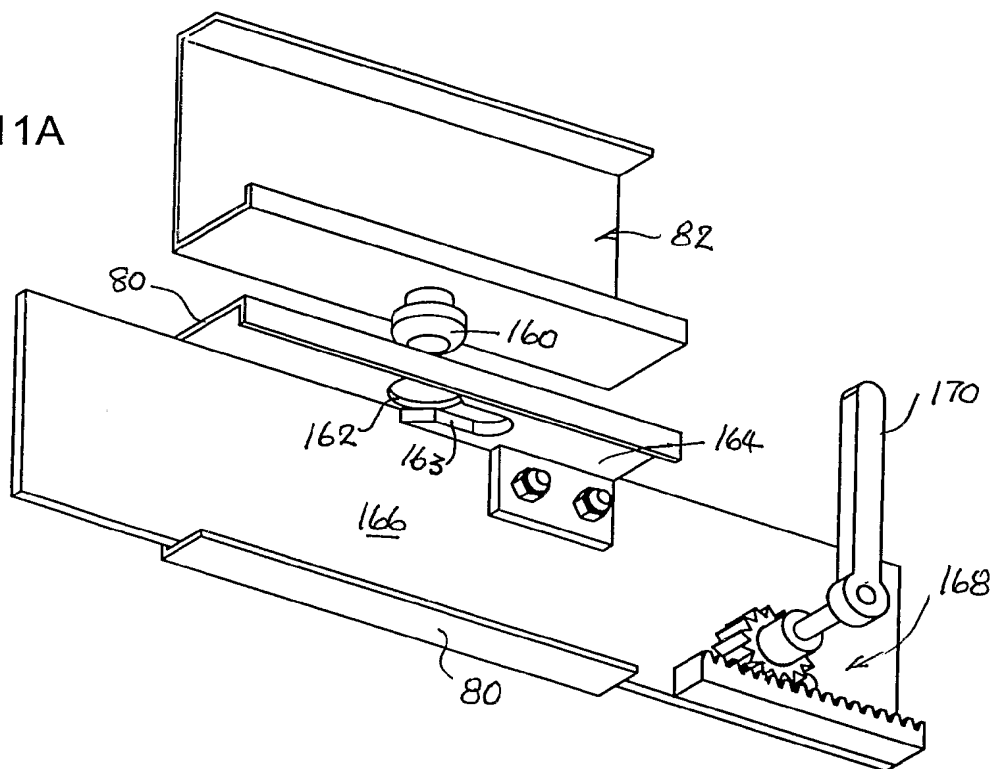

# INTERNATIONAL SEARCH REPORT

International application No.  
**PCT/AU2003/001540**

<b>A. CLASSIFICATION OF SUBJECT MATTER</b>					
Int. Cl. <sup>7</sup> : A61G 10/02, 10/00					
According to International Patent Classification (IPC) or to both national classification and IPC					
<b>B. FIELDS SEARCHED</b>					
Minimum documentation searched (classification system followed by classification symbols)					
Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched					
Electronic data base consulted during the international search (name of data base and, where practicable, search terms used) DWPI - IPC A61G 10/-, A62B 31/- and keywords ( chamber, hyperbaric, seat and similar terms); USPTO & Espace with similar keywords to those above					
<b>C. DOCUMENTS CONSIDERED TO BE RELEVANT</b>					
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.			
A	Derwent Abstract Accession No. 1999-608945/52, Class P33 S05, RU 2112486 C1 (LAZURIT STOCK CO) 10 June 1998 English abstract	1-17			
A	Derwent Abstract Accession No. 96-516747/51, Class P33, RU 2056825 C1 (LAVOHKIN RES PRODN) 27 March 1996 English abstract	1-17			
A	US 5645578 A (DAFFER et al) 8 July 1997 See abstract and figures	1-17			
<input checked="" type="checkbox"/> Further documents are listed in the continuation of Box C <input checked="" type="checkbox"/> See patent family annex					
<table style="width: 100%; border: none;"> <tr> <td style="width: 33%; vertical-align: top;"> <p>* Special categories of cited documents:</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier application or patent but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> </td> <td style="width: 33%; vertical-align: top;"> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</p> <p>"&amp;" document member of the same patent family</p> </td> <td style="width: 33%;"></td> </tr> </table>			<p>* Special categories of cited documents:</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier application or patent but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p>	<p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</p> <p>"&amp;" document member of the same patent family</p>	
<p>* Special categories of cited documents:</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier application or patent but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p>	<p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</p> <p>"&amp;" document member of the same patent family</p>				
Date of the actual completion of the international search 16 January 2004		Date of mailing of the international search report 22 JAN 2004			
Name and mailing address of the ISA/AU AUSTRALIAN PATENT OFFICE PO BOX 200, WODEN ACT 2606, AUSTRALIA E-mail address: pct@ipaustalia.gov.au Facsimile No. (02) 6285 3929		Authorized officer  <b>STEPHEN CLARK</b> Telephone No : (02) 6283 2781			

# INTERNATIONAL SEARCH REPORT

International application No.  
**PCT/AU2003/001540**

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 6352078 B1 (HARVEY et al) 5 March 2002 See abstract and figures	1-17
A	US 5327904 A (HANNUM) 12 July 1994 See abstract and figures	1-17
A	US 6016803 A (VOLBERG et al) 25 January 2000 See abstract and figures	1-17
A	US 5398678 A (GAMOW) 21 March 1995 See abstract and figures	1-17
A	WO 01/62324 A1 (SHUSTERMAN) 30 August 2001 See abstract and figures	1-17

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/AU2003/001540

This Annex lists the known "A" publication level patent family members relating to the patent documents cited in the above-mentioned international search report. The Australian Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

Patent Document Cited in Search Report		Patent Family Member					
RU	2112486	NONE					
RU	2056825	NONE					
US	5645578	AU	41079/96	CN	1164180	EP	792120
		WO	96/14792				
US	6352078	NONE					
US	5327904	NONE					
US	6016803	AU	50217/99	WO	00/04859		
US	5398678	EP	277787	EP	469071	JP	63302847
		US	4974829	US	5109837	US	5360001
		WO	90/12556				
WO	01/62324	AU	30465/01	CA	2400140	EP	1259278
		US	2003205230				
END OF ANNEX							